Name:	**mansour, abd al karem**			
ID:	407040	Exam Date:	12/16/2019	CZMI
DOB:	9/21/1967	Exam Time:	11:07 AM	
Gender:	Male	Technician:	Operator, Cirrus	
Doctor:		Signal Strength:	0/10	

Macula Thickness : Macular Cube 512x128

OD ● ○ OS

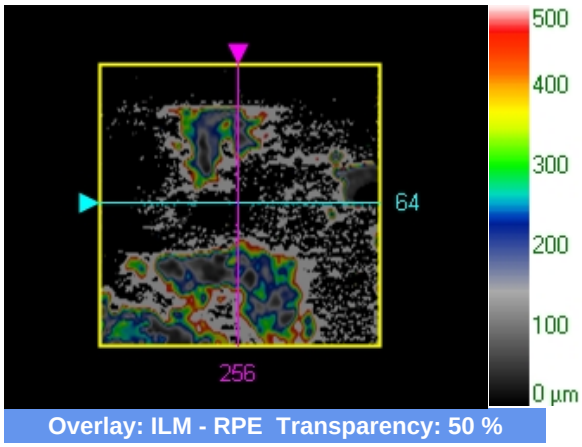

Overlay: ILM - RPE Transparency: 50 %

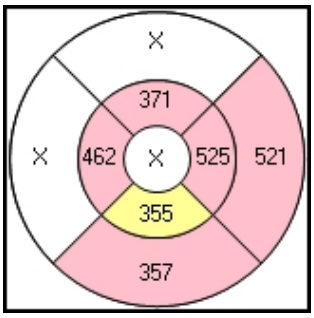

ILM-RPE Thickness (µm)

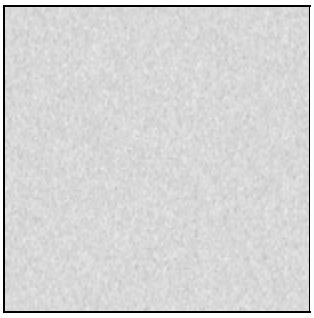

Fovea: Fovea not found

High-definition mode

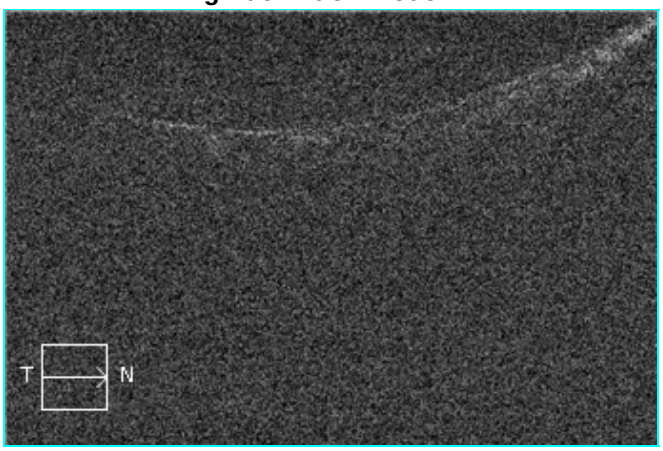

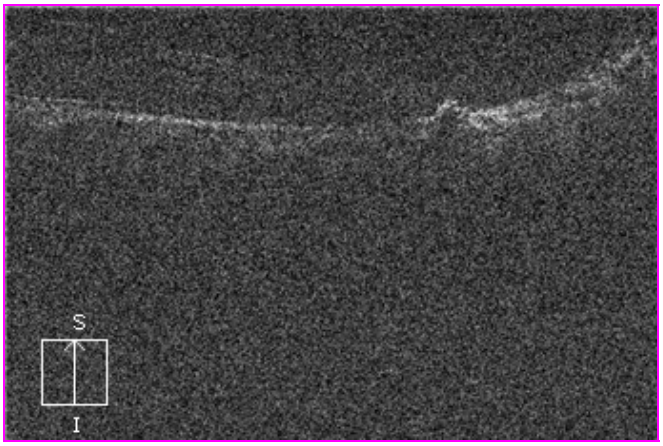

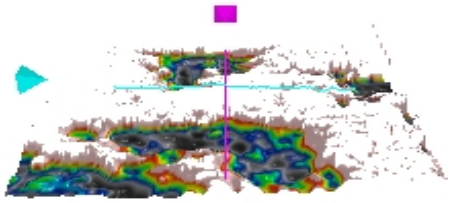

ILM - RPE

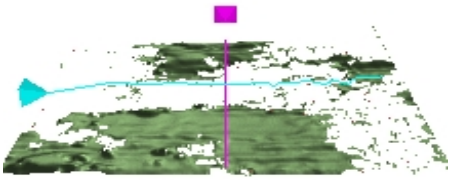

ILM

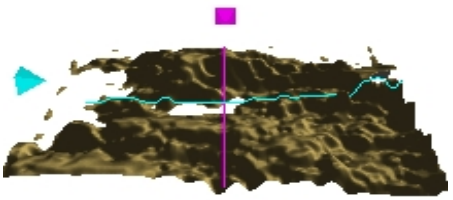

RPE



	Central Subfield Thickness (µm)	Cube Volume (mm³)	Cube Average Thickness (µm)
ILM - RPE	0	8.6	238

Comments

Doctor's Signature

SW Ver: 5.2.0.210
Copyright 2011
Carl Zeiss Meditec, Inc
All Rights Reserved